


Ordering Information

- Guidewire compatibility: 0.014"/ 0.018"
- Catheter length: B - 90cm; C - 135cm; D - 150cm

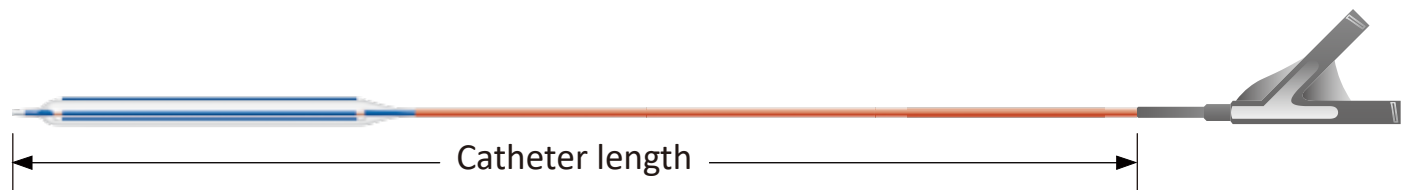

Compatible Introducer Sheath		Balloon Length							Guidewire OD(inch)
		20mm	40mm	60mm	80mm	100mm	120mm	150mm	
Balloon Diameter	5Fr	DKL14-2520B/C/D	DKL14-2540B/C/D	DKL14-2560B/C/D	DKL14-2580B/C/D	DKL14-25100B/C/D	DKL14-25120B/C/D	DKL14-25150B/C/D	0.014"
	6Fr	DKL14-3020B/C/D	DKL14-3040B/C/D	DKL14-3060B/C/D	DKL14-3080B/C/D	DKL14-30100B/C/D	DKL14-30120B/C/D	DKL14-30150B/C/D	
	7Fr	DKL14-3520B/C/D	DKL14-3540B/C/D	DKL14-3560B/C/D	DKL14-3580B/C/D	DKL14-35100B/C/D	DKL14-35120B/C/D	DKL14-35150B/C/D	
		DKL18-4020B/C/D	DKL18-4040B/C/D	DKL18-4060B/C/D	DKL18-4080B/C/D	DKL18-40100B/C/D	DKL18-40120B/C/D	DKL18-40150B/C/D	
		DKL18-4520B/C/D	DKL18-4540B/C/D	DKL18-4560B/C/D	DKL18-4580B/C/D	DKL18-45100B/C/D	DKL18-45120B/C/D	DKL18-45150B/C/D	0.018"
		DKL18-5020B/C/D	DKL18-5040B/C/D	DKL18-5060B/C/D	DKL18-5080B/C/D	DKL18-50100B/C/D	DKL18-50120B/C/D	DKL18-50150B/C/D	
		DKL18-5520B/C/D	DKL18-5540B/C/D	DKL18-5560B/C/D	DKL18-5580B/C/D	DKL18-55100B/C/D	DKL18-55120B/C/D	DKL18-55150B/C/D	
		DKL18-6020B/C/D	DKL18-6040B/C/D	DKL18-6060B/C/D	DKL18-6080B/C/D	DKL18-60100B/C/D	DKL18-60120B/C/D	DKL18-60150B/C/D	
		DKL18-6520B/C/D	DKL18-6540B/C/D	DKL18-6560B/C/D	DKL18-6580B/C/D	DKL18-65100B/C/D	DKL18-65120B/C/D	DKL18-65150B/C/D	
		DKL18-7020B/C/D	DKL18-7040B/C/D	DKL18-7060B/C/D	DKL18-7080B/C/D	DKL18-70100B/C/D	DKL18-70120B/C/D	DKL18-70150B/C/D	

- Nominal Pressure: 10 atm (All Models)
- Rated Burst Pressure: 14 atm (All Models)



DK Medical Technology Co.,Ltd.
☎ +86-512-81880801
✉ cs@dkmedtech.com
📍 Unit #5 Xinhong Park, No. 9 West Suhong Road, Suzhou



Precise Dilatation, Minimized Complication



188
Patients
1:1 RCT


14
Centers
in China




D·Kutting™ LL
PTA Scoring Balloon Dilatation Catheter

Achievement of Optimal PTA in Percent

Percentage of PTA cases in which <30% diameter stenosis without a flow limiting dissection (NHLBI grading: D-F).

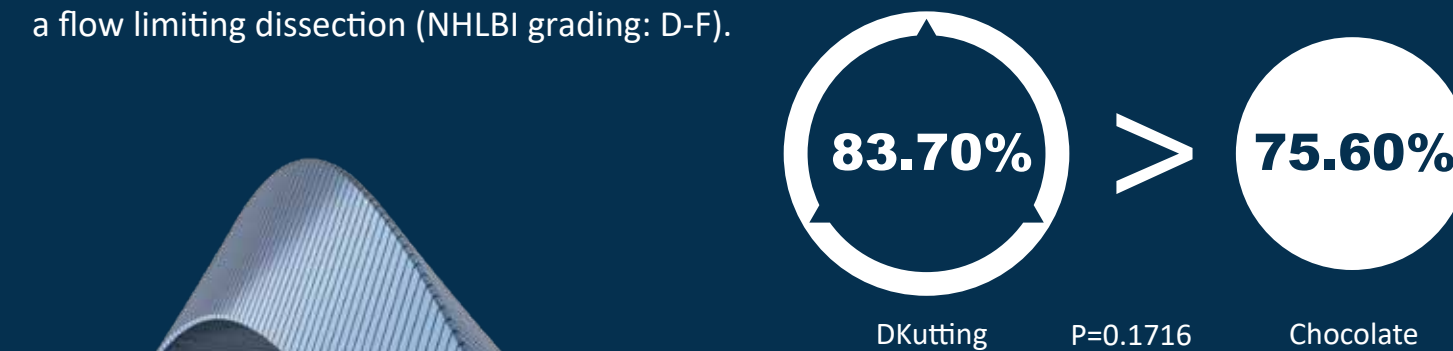

Secondary Outcome Measures

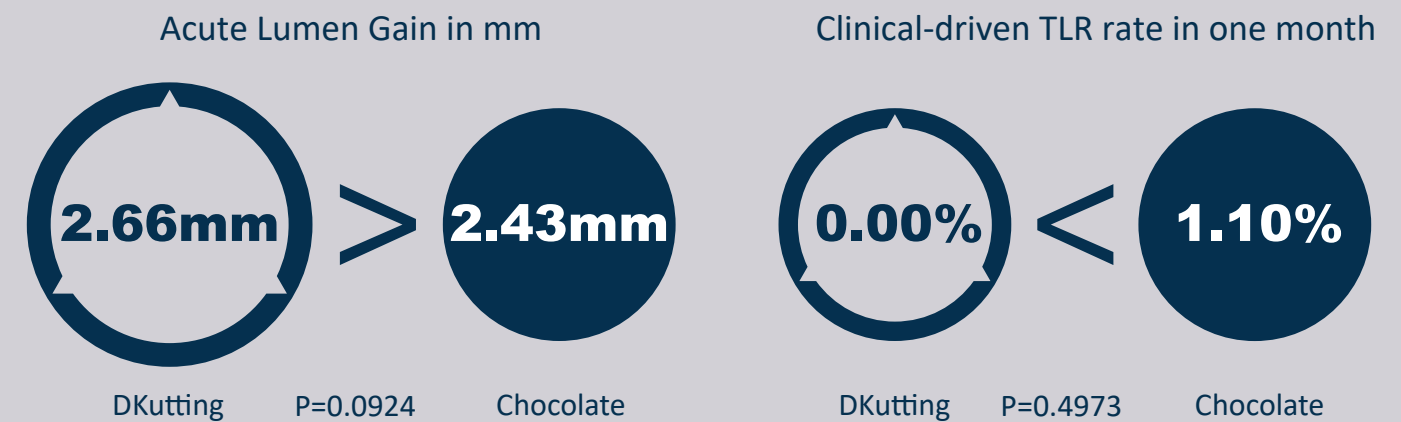


	DKutting LL	Chocolate	P-Value
Optimal PTA (CTO lesions)	83.1%	69.4%	0.0940
Total number of 1-month SAE	3	14	0.0034
Bail-out stenting %	26.60%	25.80%	0.9023
Residual stenosis %	27.79%	30.87%	0.0212
Flow-limiting dissection (NHLBI Grade:D-F)	3.30%	4.40%	NA

A Multicenter, Prospective, Randomized Controlled Trial to Evaluate the Efficacy and Safety of DKutting Balloon Versus Chocolate Balloon in the Treatment of Femoral and Popliteal Artery Stenosis (DELTA)
ClinicalTrials.gov ID NCT05608655




Triangular Scoring Elements

Highly focused force transmission




Every 120° Distributed Scoring Elements

Focused, uniform, controlled dilation



Nitinol Coilwire Scoring Elements

Conforms naturally to vascular curvature



Comprehensive Product Models

- Suitable for lower extremity arteries
- Balloon diameter: 2.5/3/3.5/4/4.5/5/5.5/6/7 mm
- Balloon length: up to 150 mm